



ADTECH
 Analog-Digital Technology, Inc.
 95 Mt. Read Blvd Suite 149
 Rochester, New York 14611 USA
 Phone 1.585.698.1845 Fax 1.585.697.0445

PDR 82 Isolated Pulse Duration Receiver Instruction Manual

1.0 INTRODUCTION

These instructions refer to the above model. Supplementary sheets are attached if the unit has special options or features. For detailed specifications, see page 4 or refer to the Data Bulletin. All ADTECH instruments are factory calibrated and supplied with a label detailing the calibration. Adjustments are normally not necessary. A simple check should be performed to verify calibration before installation to ensure that it matches the field requirement.

2.0 GENERAL DESCRIPTION

The ADTECH PDR 82 is an Isolated Pulse Duration Receiver that accepts a pulse duration or pulse cycle signals of 0.1 to 300 seconds duration and converts it into any of the standard control signal outputs such as 4-20 ma dc.

The input is electrically isolated from the output and the power supply by 600 volts ac or 1000 vdc peak on AC powered and isolated DC powered units. Power option P-1 Non-Isolated 24 vdc provides negative output signal and negative DC power common rail connection.

The output is a true current source and provides process signals such as 4-20 ma, 0-1 ma, 0-10 ma, 1-5 ma and 10-50 ma dc or alternatively, a voltage signal of 5 vdc full scale. Other current and voltage **Inputs/Outputs (I/O)** are available as specified on the Data Bulletin.

3.0 INSTALLATION

The instrument is supplied in a general purpose enclosure as standard. NEMA 4, 7 or 12 and plug in chassis enclosures are optionally available. Installation area/location must agree with the supplied instruments including operating temperature and ambient conditions.

Mounting

Refer to the appropriate outline drawing for mounting and clearance dimensions. The instrument is surface mounted with two #10-32 screws on 8.00 inch centers.

Electrical Connections

The wire used to connect the instrument to the control system **I/O** should be a twisted pair(s) and sized according to normal practice. Shielded cable is not normally necessary (if used, the shield must be grounded at the input negative of the ADTECH instrument and left floating at the sensor).

A 12 position barrier terminal block with #6-32 screws and 3/8" spacing is provided for **I/O** and power connection. A housing ground terminal marked G is also provided.

Controls

Multiturn ZERO, SPAN and PERIOD controls are provided to calibrate the instrument. The multiturn controls are accessible through the instrument front panel and are clearly marked for ease of use.


4.0 MAINTENANCE

These instruments are electronic and require no maintenance except periodic cleaning and calibration verification. If the unit appears to be mis-operating it should be checked as installed per section 6.0 or removed for a bench check per sections 6.0-7.0. MOST problems are traced to field wiring and/or associated circuits. If the problem appears to be with the instrument, proceed to sections 6.0 and 7.0.

5.0 CONNECTIONS

Standard connections are shown below and on the instrument face plate, Data Bulletin or on attached supplementary sheets.

CAUTION: NO customer connection to Terminal No. 4

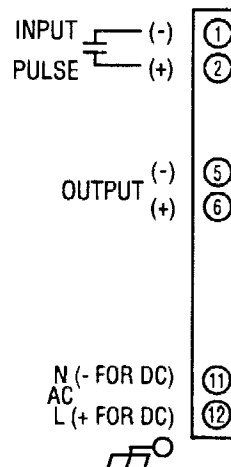

6.0 CALIBRATION

To perform a calibration check or re-calibration of the instrument follow this procedure.

- A. Make sure the unit I/O wiring is properly connected and that the correct power source per the label is also connected. The instrument must be at normal power for a minimum of 2 minutes before proceeding to B.
- B. The input signal source function generator must be adjustable from 0 to 100% in steps of 10% or at least 25%. The source(s) should be either precalibrated or an accurate meter must be used to monitor the input(s).
- C. The output may be monitored either as a direct voltage for a voltage output signal or as a current that can be represented as a voltage across a resistor shunt.
- D. Look up values of T(sec) and N from Input Table on page 3. Connect a frequency meter across terminals 4(+) and 5. Adjust control #3 to obtain $\text{freq} = \frac{8192N}{T(\text{sec})}$ Hz.
- E. Set the input source to minimum input value and adjust the multiturn potentiometer marked ZERO to provide the minimum calibrated output (e.g.) $4.00 \text{ ma} \pm 0.01 \text{ ma dc}$.
- F. Set the input source to maximum value and adjust the multiturn potentiometer marked SPAN to provide the maximum calibrated output (e.g.) $20.00 \text{ ma} \pm 0.01 \text{ ma dc}$.
- G. Repeat steps D and E until readings are within calibration.
- H. The instrument should now be checked at 25-50-75% of span minimum.
- I. This completes the calibration.

NOTE:

If recalibration to a different input and/or output signal is required, proceed to the tables listed below and under section 8.0.

For Voltage Pulse Input: J2 = A, Delete R61 (4.7 k Ω)

For Contact Closure Input: J2 = B, Keep R61 (4.7 k Ω)

7.0 FIELD TROUBLE SHOOTING GUIDE

This section offers a simple, first level trouble-shooting aid for an apparent instrument malfunction.

SYMPTOM CORRECTIVE ACTION

- | | |
|-----------|---|
| No output | <ol style="list-style-type: none"> 1. Check the input and output connections carefully. 2. Check that the power supply polarity is correct and that power is present on the instrument terminals. 3. Check that the input source(s) is correct and that it changes magnitude between zero and full scale values when so adjusted. 4. If the output is a current signal (4-20 ma, etc.), make sure the output loop is complete and that the correct meter range is selected. |
|-----------|---|

All external checks are complete. Problem seems to be internal.

The following information is provided for a qualified technician or serviceman as check points for use in internal troubleshooting.

| <u>CHECKPOINT/ COMPONENT</u> | <u>VOLTAGE/ RANGE</u> |
|----------------------------------|----------------------------|
| (across) C11 | $11 \pm 0.6 \text{ vdc}$ |
| (across) C24 | $11 \pm 0.6 \text{ vdc}$ |
| (across) C8 | $0.2 - 1 \text{ vdc}$ |
| (across) C16 | $26 \pm 4 \text{ vdc}$ |
| (across) C9 | $12 \pm 0.6 \text{ vdc}$ |
| (across) D10 | $6.9 \pm 0.35 \text{ vdc}$ |

8.0 TABLES, PCB LAYOUT

INPUT TABLE

| PERIOD T SEC | J10 | J11 | J13 | J14 | J15 | N (RATIO) |
|-----------------|-----|-----|-----|-----|-----|--------------|
| 0.95 - 1.9 | A | A | A | A | B | 1 |
| 1.9 - 3.8 | A | A | A | B | B | 2 |
| 3.8 - 7.6 | A | A | B | A | B | 4 |
| 7.6 - 15.2 | A | A | B | B | B | 8 |
| 15.2 - 30.4 | A | B | A | A | B | 16 |
| 30.4 - 60.8 | A | B | A | B | B | 32 |
| 60.8 - 122 | A | B | B | A | B | 64 |
| 122 - 244 | A | B | B | B | B | 128 |
| 244 - 488 | B | A | A | A | B | 256 |

A & B are two selectable positions of a jumper

OUTPUT TABLE

| OUTPUT SIGNAL FULL SCALE | OUTPUT SHUNT RL | FEEDBACK RES RF |
|-----------------------------|--------------------|--------------------|
| 50 ma dc | NONE | 20 ohm |
| 20 ma dc | NONE | 49.9 ohm |
| 10 ma dc | NONE | 100 ohm |
| 1 ma dc | NONE | 1K ohm |
| 10 vdc | 604 ohm, 1/4 W | 49.9 ohm |
| 5 vdc | 250 ohm, 1/4 W | 49.9 ohm |


All selected resistors are 1%, M.F., 1/4 W, 50 PPM.

NOTE A: Components as shown may or may not be present on the p.c. board due to design updates or options.

TABLE 3

| INPUT | OUTPUT | J6 | J8 |
|------------|------------|----|----|
| ZERO BASED | ZERO BASED | B | A |
| ZERO BASED | LIVE ZERO | B | B |
| LIVE ZERO | ZERO BASED | A | A |
| LIVE ZERO | LIVE ZERO | A | B |

PDR 82 RL = R51 RF = R15

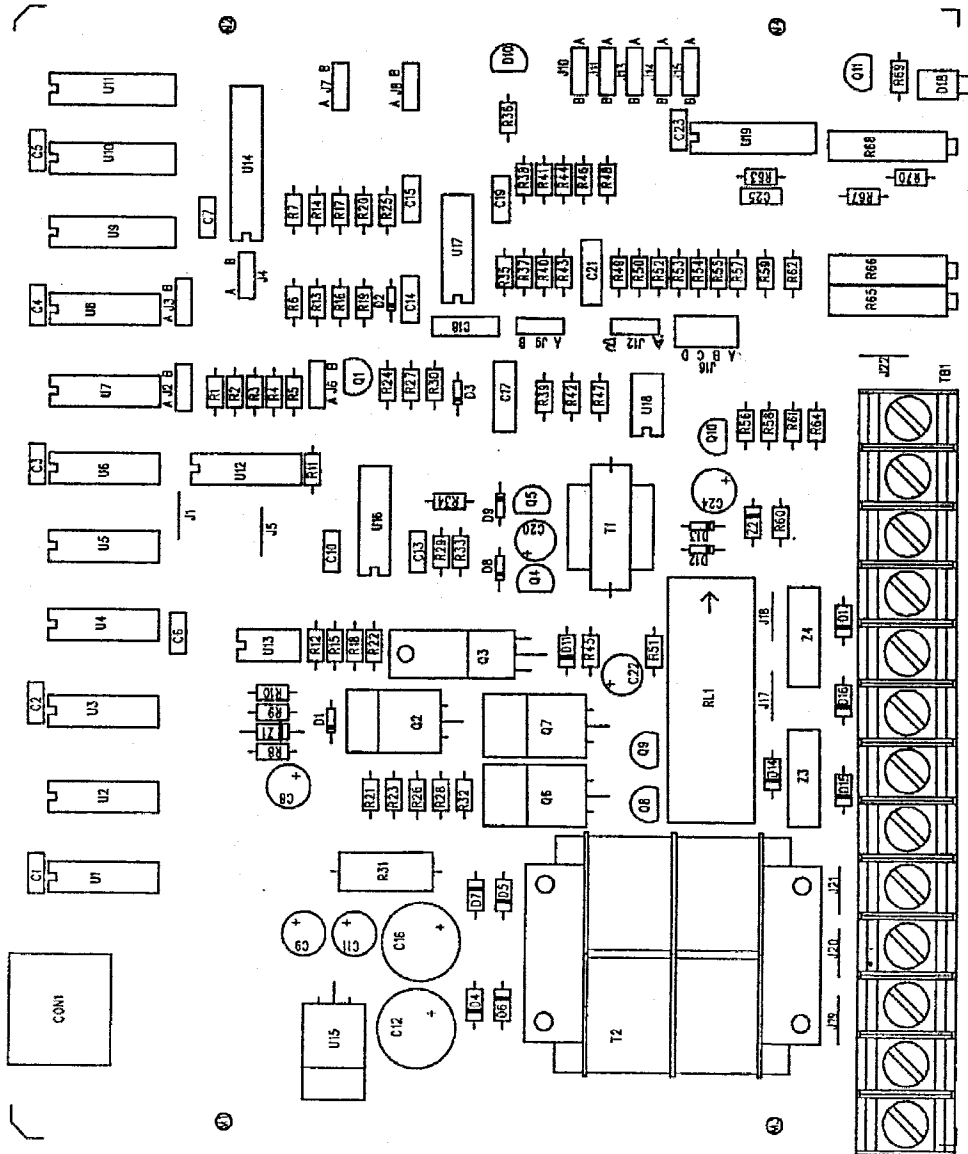

9.0 SPECIFICATIONS

INPUT/OUTPUT

INPUT SIGNALS

- Voltage:** 24 vdc maximum into 500 W minimum
 - Contact:** Dry, 10 va @ 24 vdc rating: Optional
 - Period:** 0.1 to 300 seconds
 - Input Ranges:**
 - 0 to 2 seconds
 - 0 to 13.33 seconds
 - 1 to 5 seconds
 - 3 to 12 seconds
 - 5 to 25 seconds
- Other Periods/Ranges: Optional

OUTPUT SIGNALS/OUTPUT DRIVE

| | AC Power | DC Power |
|----------------|--------------------|--------------------|
| a. 4-20 ma dc | 0-1000 ohms max. | 0-900 ohms max. |
| b. 10-50 ma dc | 0-400 ohms max. | 0-350 ohms max. |
| c. 0-1 ma dc | 0-20,000 ohms max. | 0-18,000 ohms max. |
| d. 1-5 vdc | 250 ohms Z out | 250 ohms Z out |
| e. 0-10 vdc | 500 ohms Z out | 500 ohms Z out |

Or zero based in the same ranges. Other voltage and currents optional.

PERFORMANCE

- Calibrated Accuracy:** $\pm 0.1\%$
- Linearity:** $\pm 0.1\%$ maximum, $\pm 0.04\%$ typical
- Repeatability:** $\pm 0.05\%$ maximum
- Temperature Stability:** $\pm 0.01\%/^{\circ}\text{F}$ maximum, $\pm 0.004\%/^{\circ}\text{F}$ typical
- Load Effect:** $\pm 0.01\%$ zero to full load
- Output Ripple:** 10 mv P/P maximum
- Response Time:** 1 cycle time
- Temperature Range:** 0° to 140°F (-18° to 60°C) operating
 -40° to 185°F (-40° to 85°C) storage
- Power Supply Effect:** $\pm 0.05\%$ for a $\pm 10\%$ power variation
- Common Mode Rejection:** 140 db @ 60 Hz
- Isolation:** Input/output/power 600 vac, 50/60 Hz, 1000 vdc for AC and isolated DC powered units

Note: All accuracies are given as a percentage of span

POWER

- 115 vac: $\pm 10\%$, 50/60 Hz, 3 watts, 0.7 Pf (standard)
- 24 vdc: $\pm 10\%$ non-isolated, 3 watts (Option P1)
- 24 vdc: $\pm 10\%$ isolated, 3 watts (Option P2)
- 48 vdc: $\pm 10\%$ isolated, 3 watts (Option P3)
- 125 vdc: Nominal (105-140 vdc) isolated, 3 watts (Option P4)
- 230 vac: $\pm 10\%$, 50/60 Hz, 3 watts, 0.7 PF (Option P5)

10.0 OUTLINE & MOUNTING

